

St. Joseph's Villa, Dundas Long term Care



Existing Currently NCS in use:

- Executone Nurse Call Station for two wings on 5th floor
- Bed Station in room and Pull card in washroom, in total 38 rooms
- Dome light outside of the room door
- Zone based buzzer on each wing

System Upgrade requirements:

- Big 42' Alarm Screen 1080P with the TTS option with the history frame
- Logging and keeping records of NCS activity for one year minimum
- Analytic Reports to send out every Monday at 08:00AM
- Automated Report of Staff Response time, from Alarm On to Canceled Alarm
- Automated Report of Alarm Summary, Total Calls and Response time in Excel format
- Automated Report of Activity per room, what rooms using system at most
- Report generated on demand: Per Wing, Per room, per group, per department
- Remove old not working master station and peripherals from it

Equipment Provided by Controlledcare:

- LCD screen 42' wall mountable and thin client over HDMI
- Advanced Controlledcare controller with 64 opto-isolated Inputs
- Alarm, Event and Reporting Management Server
- Mini switch 5 ports on the floor


Solution Implemented by Controlledcare:

- Automated Reports per requirement, scheduled every Monday at 08:00AM, in total 3
- Analytic on request with the filtering and sorting options, exported to PDF or Excel
- Remote access to Web Portal through any type of browser
- Alarms Live Panel Screen Super HD with the history frame


Benefits of provided solution:

- Satisfied government officer requirements in evidence and archive
- Better staff management and reduced operational cost
- Full evidence of staff and patient care in case of future disputes
- No more expensive maintenance contract and looking for parts and repair
- No more old legacy equipment


OLD EQUIPMENT:

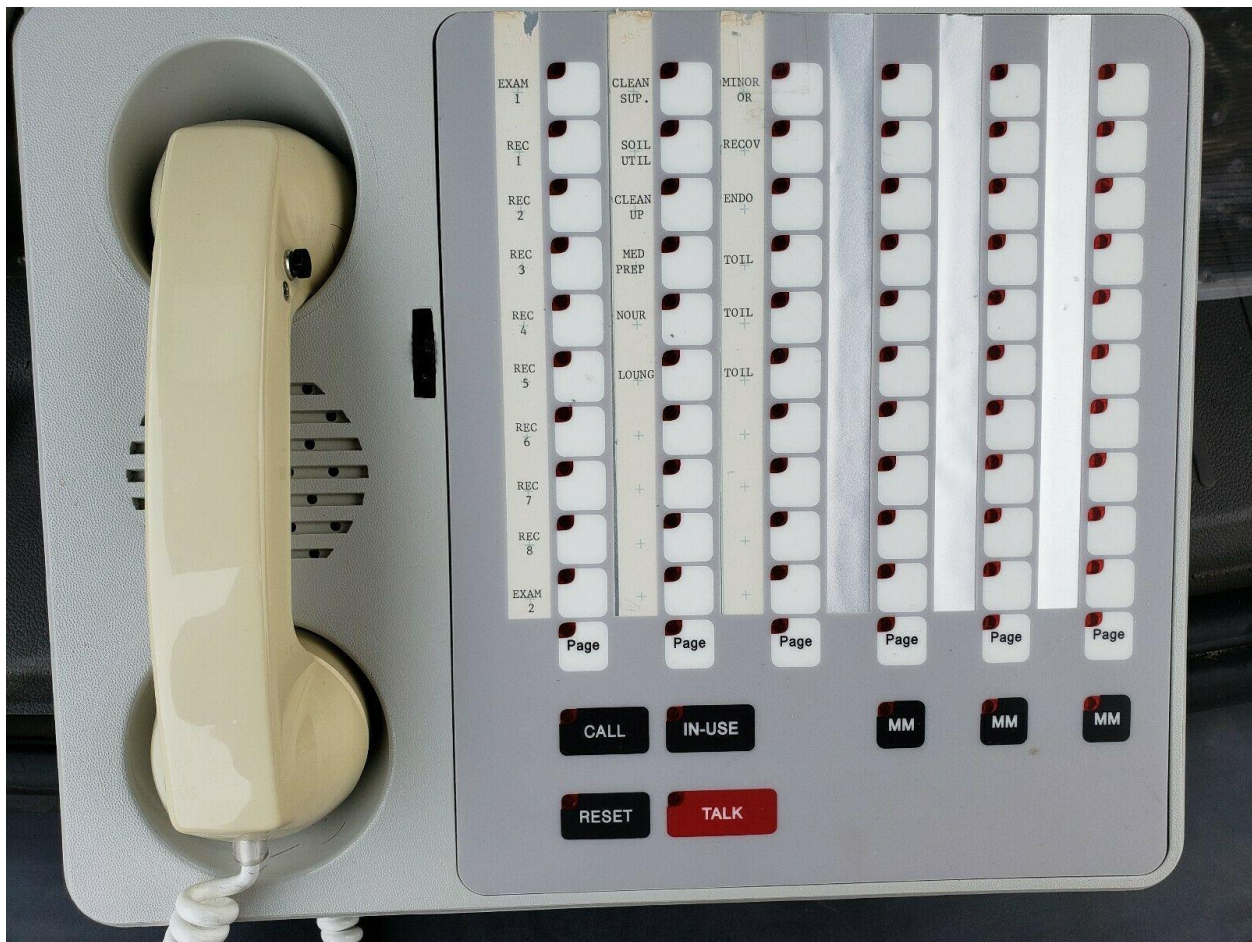

NEW EQUIPMENT:

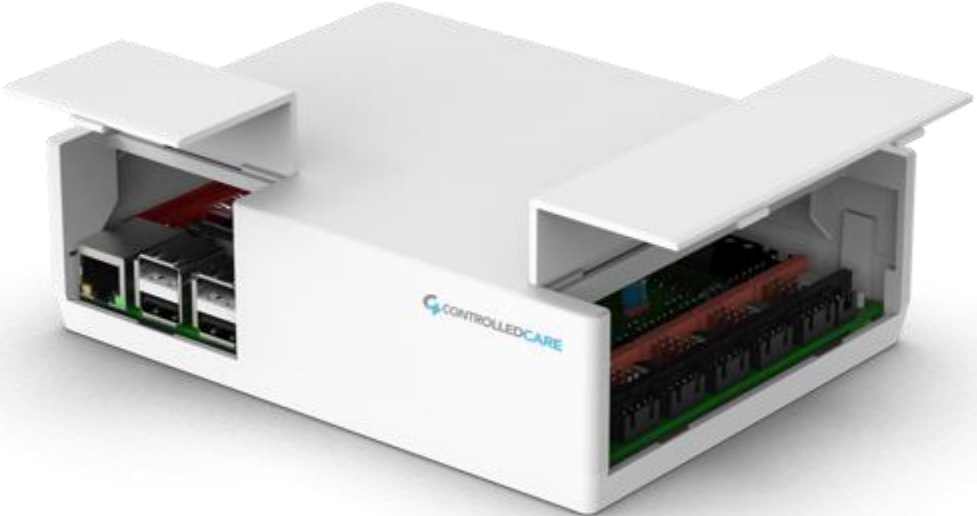

Friday, August 16, 2019 - Thursday, August 29, 2019

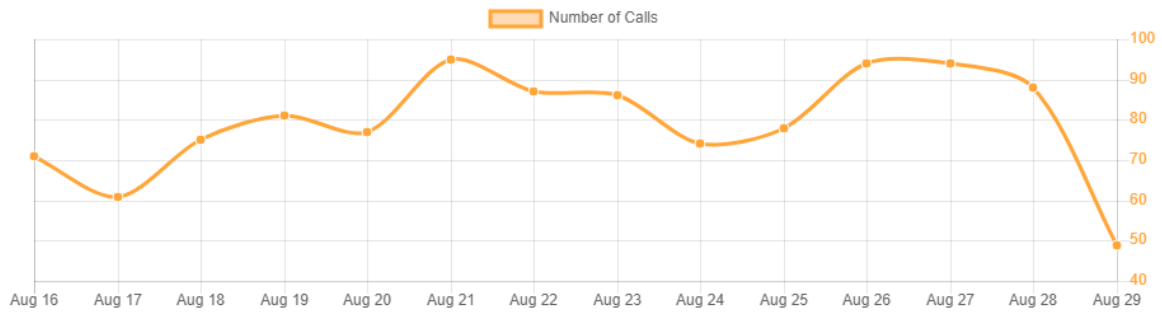


Control Button	Floor #	Department	Room #	Bed #	Total Calls
Bed Cord	5	Fifth Floor	E525		112
Bed Cord	5	Fifth Floor	E543		90
Bed Cord	5	Fifth Floor	E527		59
Bed Cord	5	Fifth Floor	N506		57
Bed Cord	5	Fifth Floor	N504		57
Bed Cord	5	Fifth Floor	N510		56
Bath Pull Cord	5	Fifth Floor	N BATH		50
Bath Pull Cord	5	Fifth Floor	E BATH		48
Bed Cord	5	Fifth Floor	E528		47
Bed Cord	5	Fifth Floor	N505		42
Bed Cord	5	Fifth Floor	E548		41
Bed Cord	5	Fifth Floor	N501		39
Bed Cord	5	Fifth Floor	E526		31
Bed Cord	5	Fifth Floor	N509		29
Bed Cord	5	Fifth Floor	E546		28
Bed Cord	5	Fifth Floor	N503		28
Bed Cord	5	Fifth Floor	E542		27
Bath Pull Cord	5	Fifth Floor	E543		25
Bed Cord	5	Fifth Floor	N522		23

Analytics Response Summary Report

Facility: Dundas Villa

Time Period: 8/23/2019 12:00 AM - 8/29/2019 12:00 AM

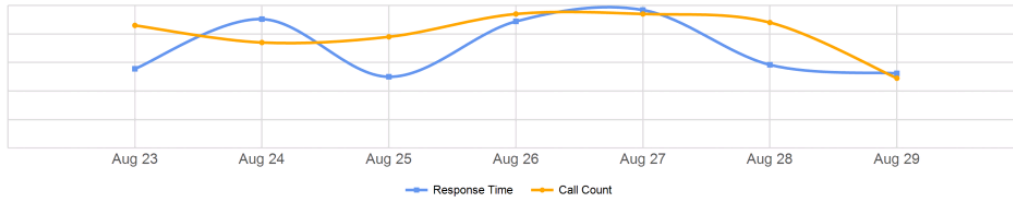

Control Button	Department	Floor #	Room #	Bed #	Total Calls	Response Time Avg.
Bath Pull Cord	Fifth Floor	5	N522		3	00h:18m:40s
Bed Cord	Fifth Floor	5	N522		10	00h:10m:23s
Bed Cord	Fifth Floor	5	N521		2	00h:08m:41s
Bath Pull Cord	Fifth Floor	5	E548		2	00h:06m:43s
Bed Cord	Fifth Floor	5	E534		4	00h:05m:05s
Bed Cord	Fifth Floor	5	E532		11	00h:04m:46s
Bed Cord	Fifth Floor	5	E546		15	00h:04m:41s
Bed Cord	Fifth Floor	5	N508		9	00h:04m:39s
Bath Pull Cord	Fifth Floor	5	N501		1	00h:04m:28s
Bed Cord	Fifth Floor	5	N506		26	00h:03m:54s
Bed Cord	Fifth Floor	5	E528		18	00h:03m:49s
Bed Cord	Fifth Floor	5	N510		38	00h:03m:41s

Master Communicator by ControlledCare.com

Page 1 of 3



- Activated: 08/29/2019 02:13:22 PM
 Canceled: 08/29/2019 02:17:23 PM
 Response: 00h:04m:01s 00h:00m:17s ago
- Activated: 08/29/2019 02:13:19 PM
 Canceled: 08/29/2019 02:17:22 PM
 Response: 00h:04m:03s 00h:00m:18s ago
- Activated: 08/29/2019 02:13:53 PM
 Canceled: 08/29/2019 02:15:10 PM
 Response: 00h:01m:17s 00h:02m:30s ago
- Activated: 08/29/2019 02:03:52 PM
 Canceled: 08/29/2019 02:05:03 PM
 Response: 00h:01m:11s 00h:12m:37s ago
- Activated: 07/12/2019 09:51:18 AM
 Canceled: 07/12/2019 09:51:27 AM
 Response: 00h:00m:09s 1156h:26m:12s ago
- ! ● Activated: 07/12/2019 09:51:14 AM
 Canceled: 07/12/2019 09:51:26 AM


- Dashboard
- Live Panel
- Device Record Test
- Analytics
- Analytics Template
- Beacon Log
- Recurring Report
- Application Config
- Admin Config
- User / Role Admin

Dundas Villa | Select Department | Select Floor

08/23/2019 - 08/29/2019

 CURRENT ALARMS 0	 NUMBER OF CALLS 514	 AVERAGE RESPONSE ... 00h:03m:05s	 TOTAL PATIENTS 0
--	---	---	--

Total Number Of Calls

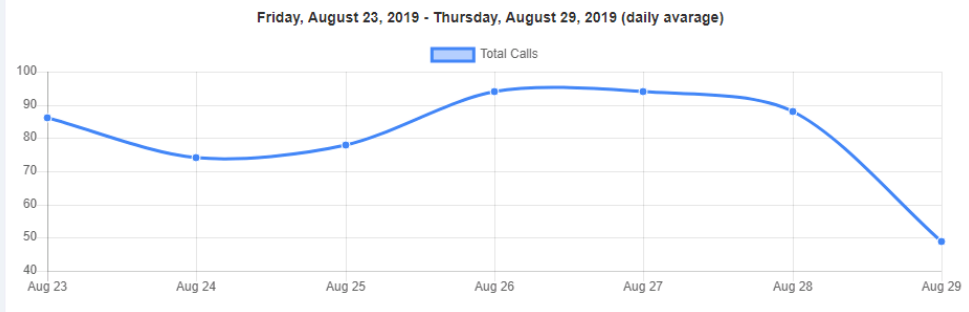

Number Of Calls By Control (Button) Type

